

BEST VIEWS: EVALUATION OF DIFFERENT NEEDLES AND ULTRASOUND MODES FOR REGIONAL ANAESTHESIA

S. Saha, J. Mukherjee

Department of Anaesthesia, Barnet General Hospital, London, UK

Barnet and Chase Farm Hospitals



NHS Trust

Chase Farm Hospital
Barnet and Chase Farm Hospital
NHS Trust

Background and Aims

- Our aim was to evaluate the image quality of the various needles and ultrasound modes available for ultrasound guided regional anaesthesia at our hospital.



Methods

- 23 anaesthetists took part in the study.
- We used a Blue Phantom and Sonosite S-Cath to compare 4 options: the B Braun Stimuplex A, B Braun hyperechogenic Stimuplex D+, Pajunk hyperechogenic Sonotap and Sonosite's multibeam enhancement (MBe) mode with the Stimuplex A.
- The image with each needle was rated as good, adequate or poor and ranked best to worst.



Results

- The Pajunk Sonotap was the overall highest rated although the MBe mode with the Stimuplex A had similar image quality.
- These were followed by the Stimuplex D+ and finally the Stimuplex A unenhanced.

Comparison rating of view

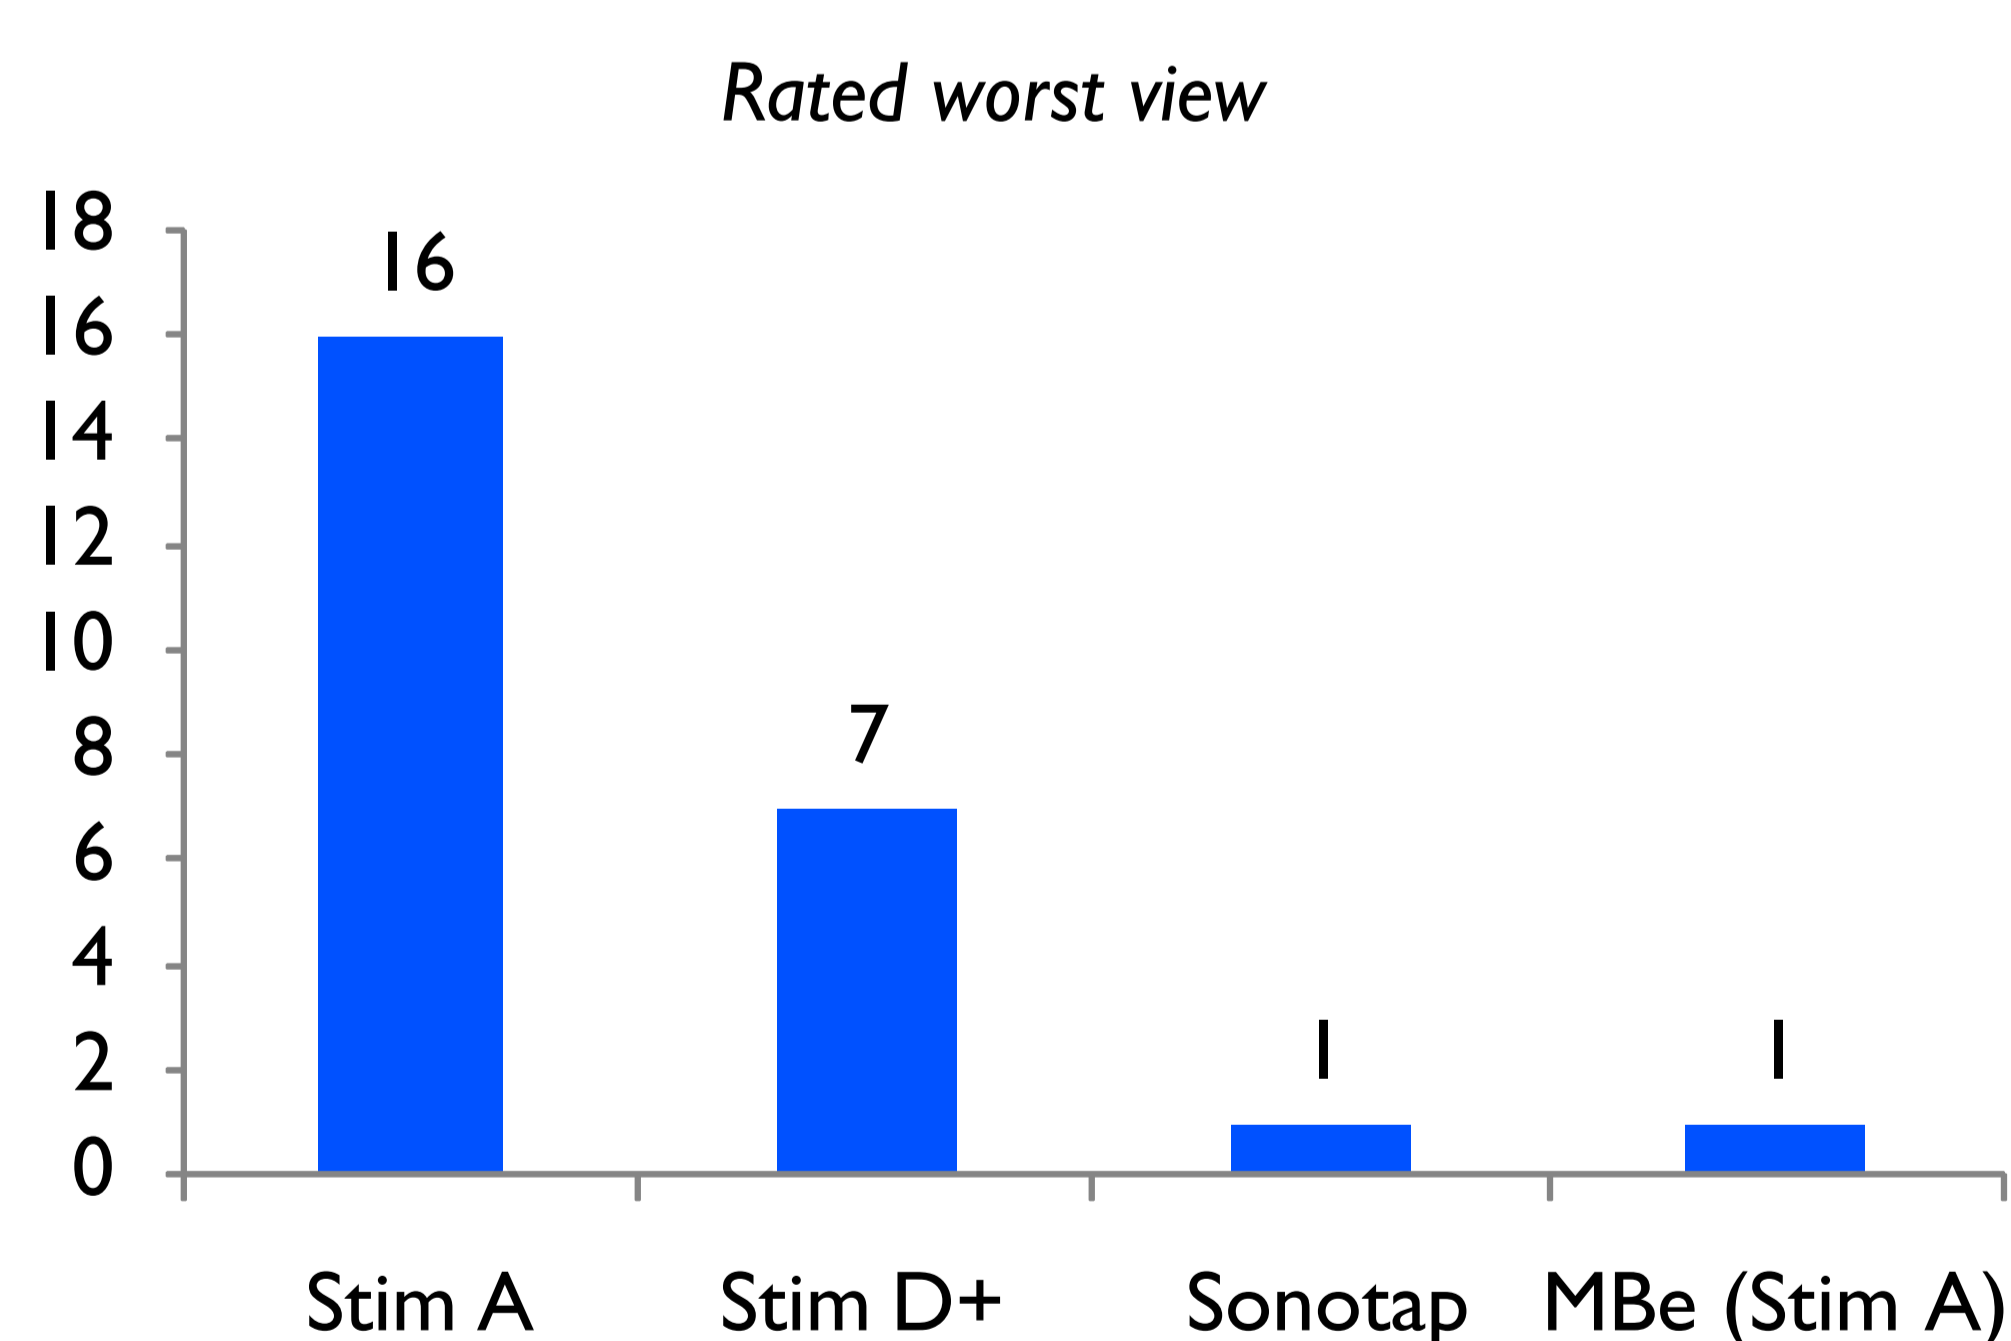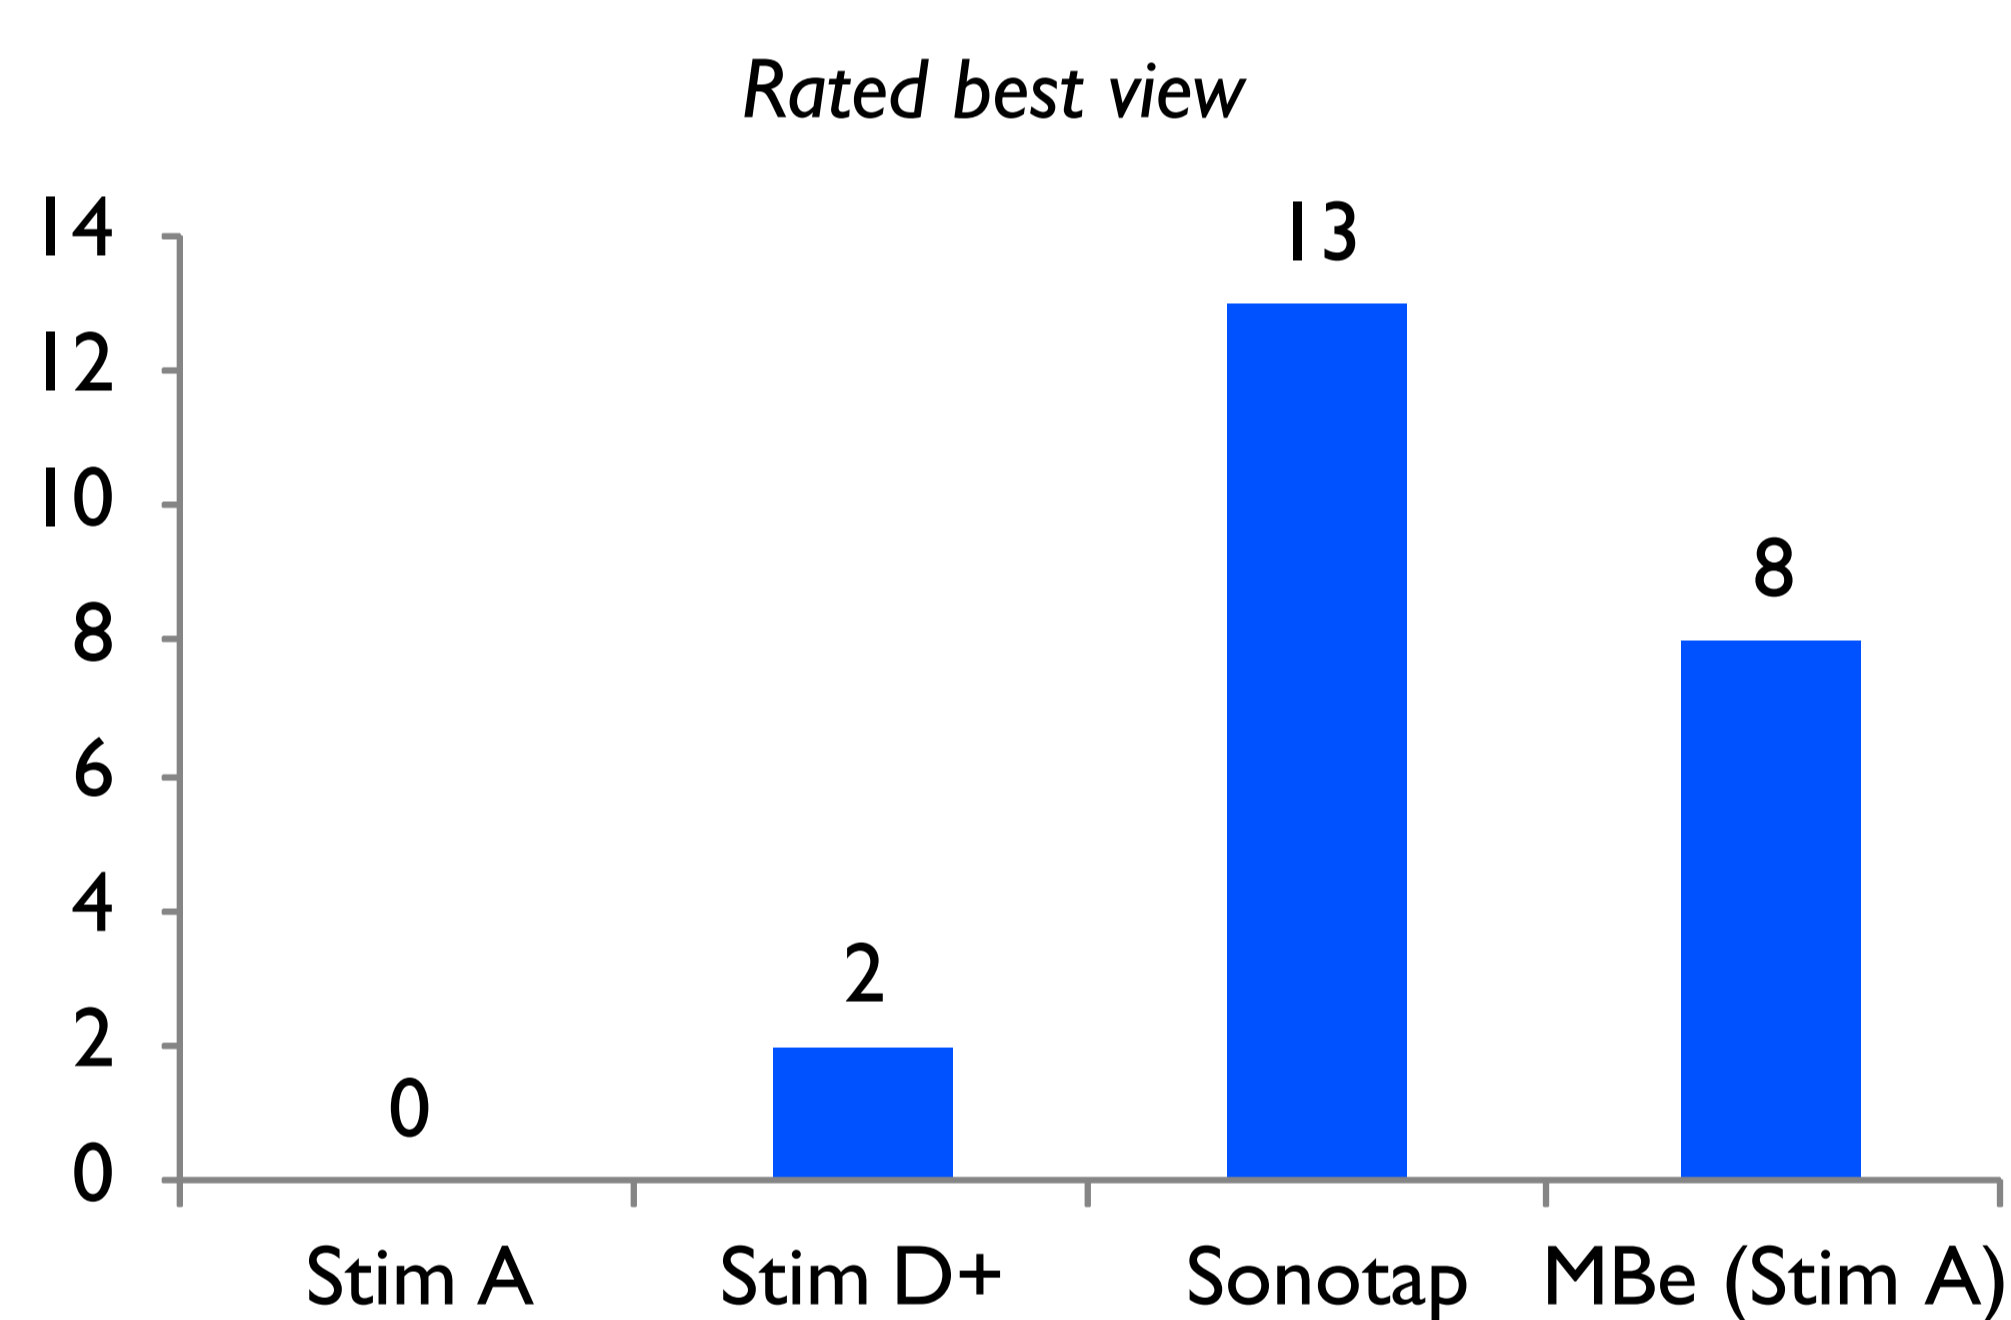

Individual rating of view

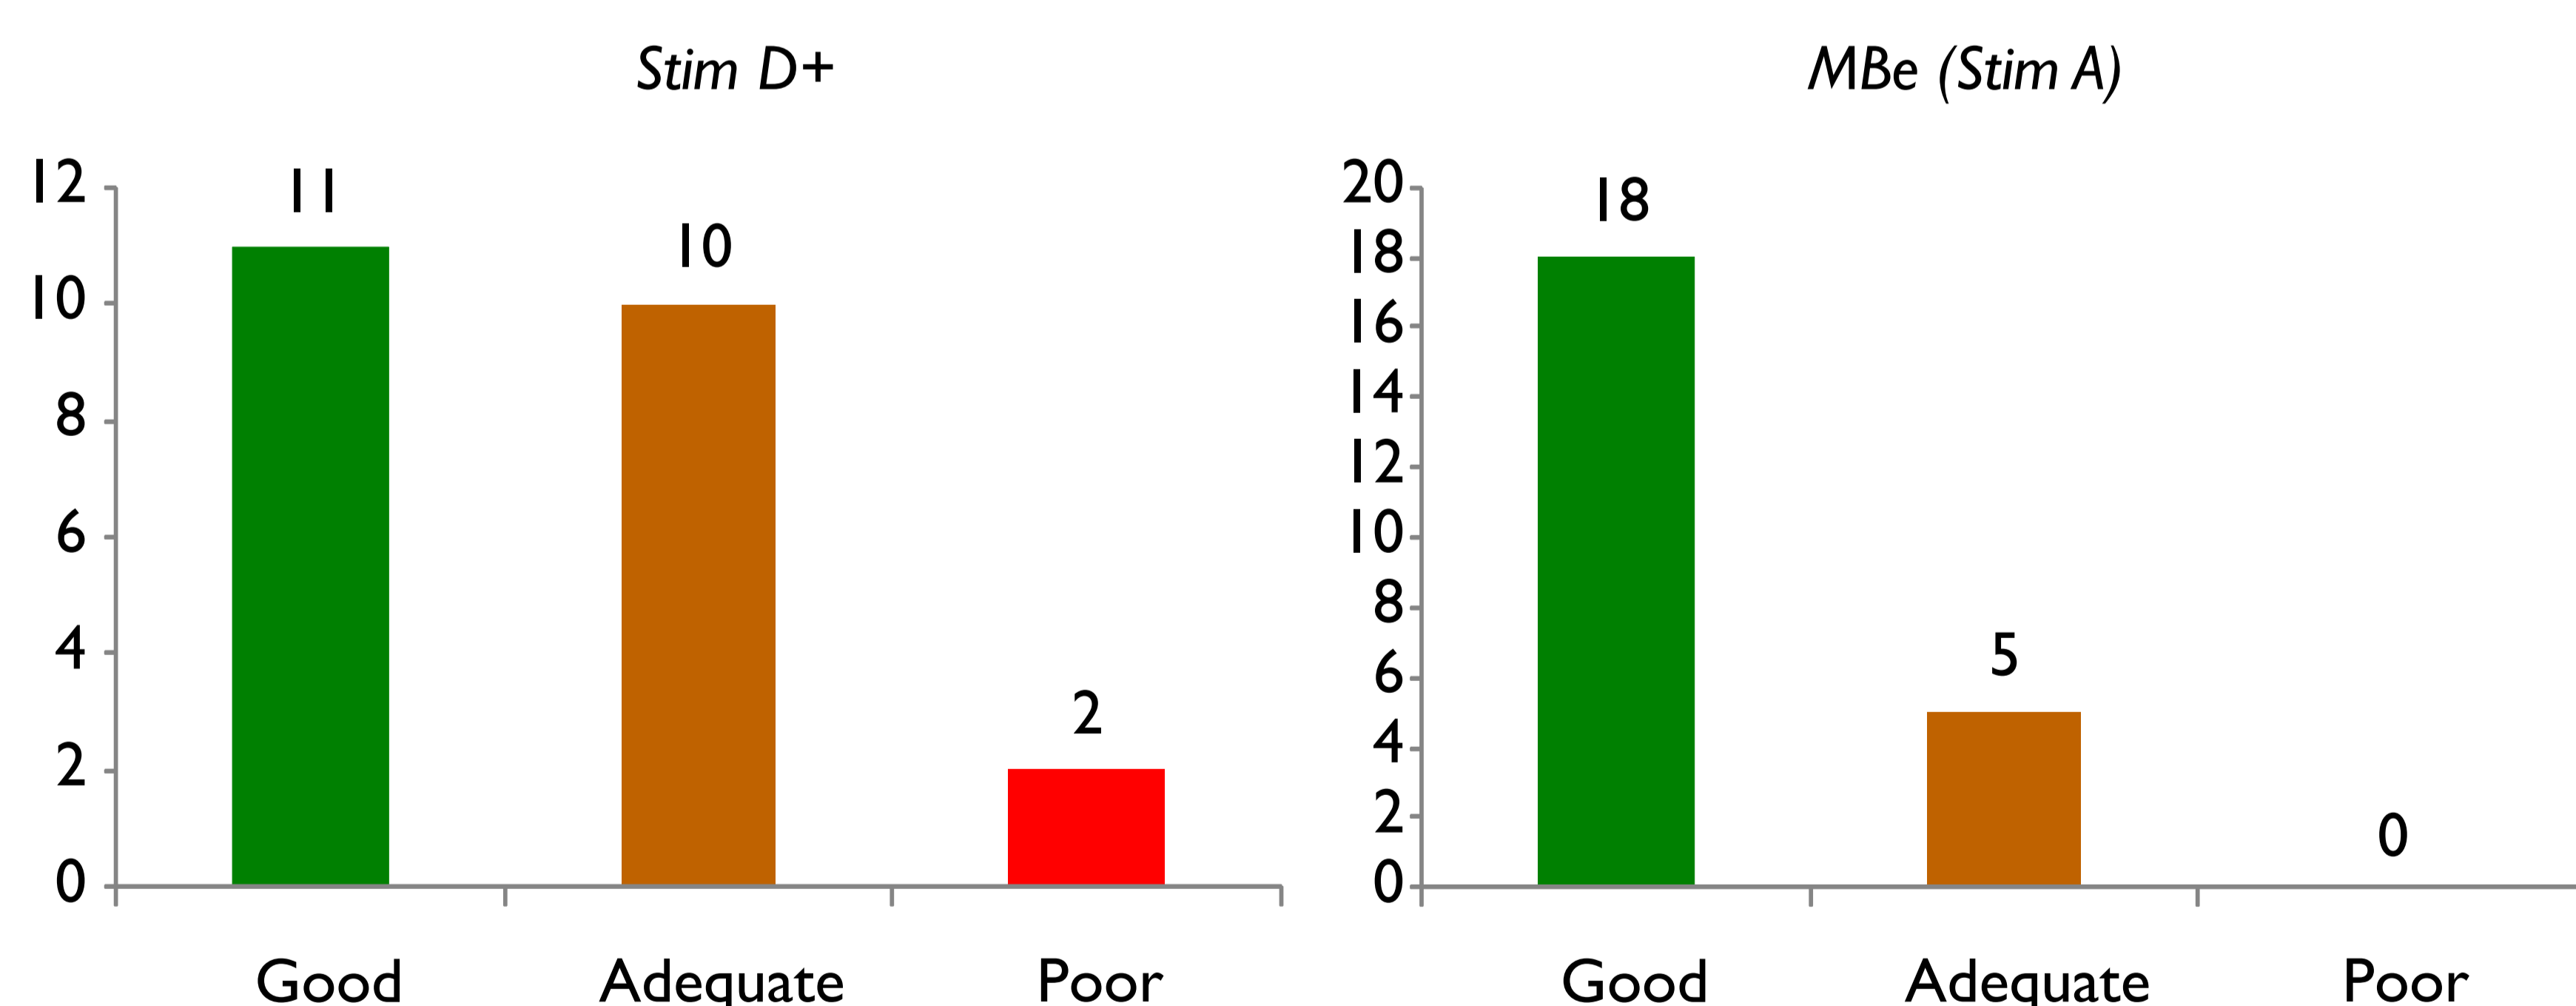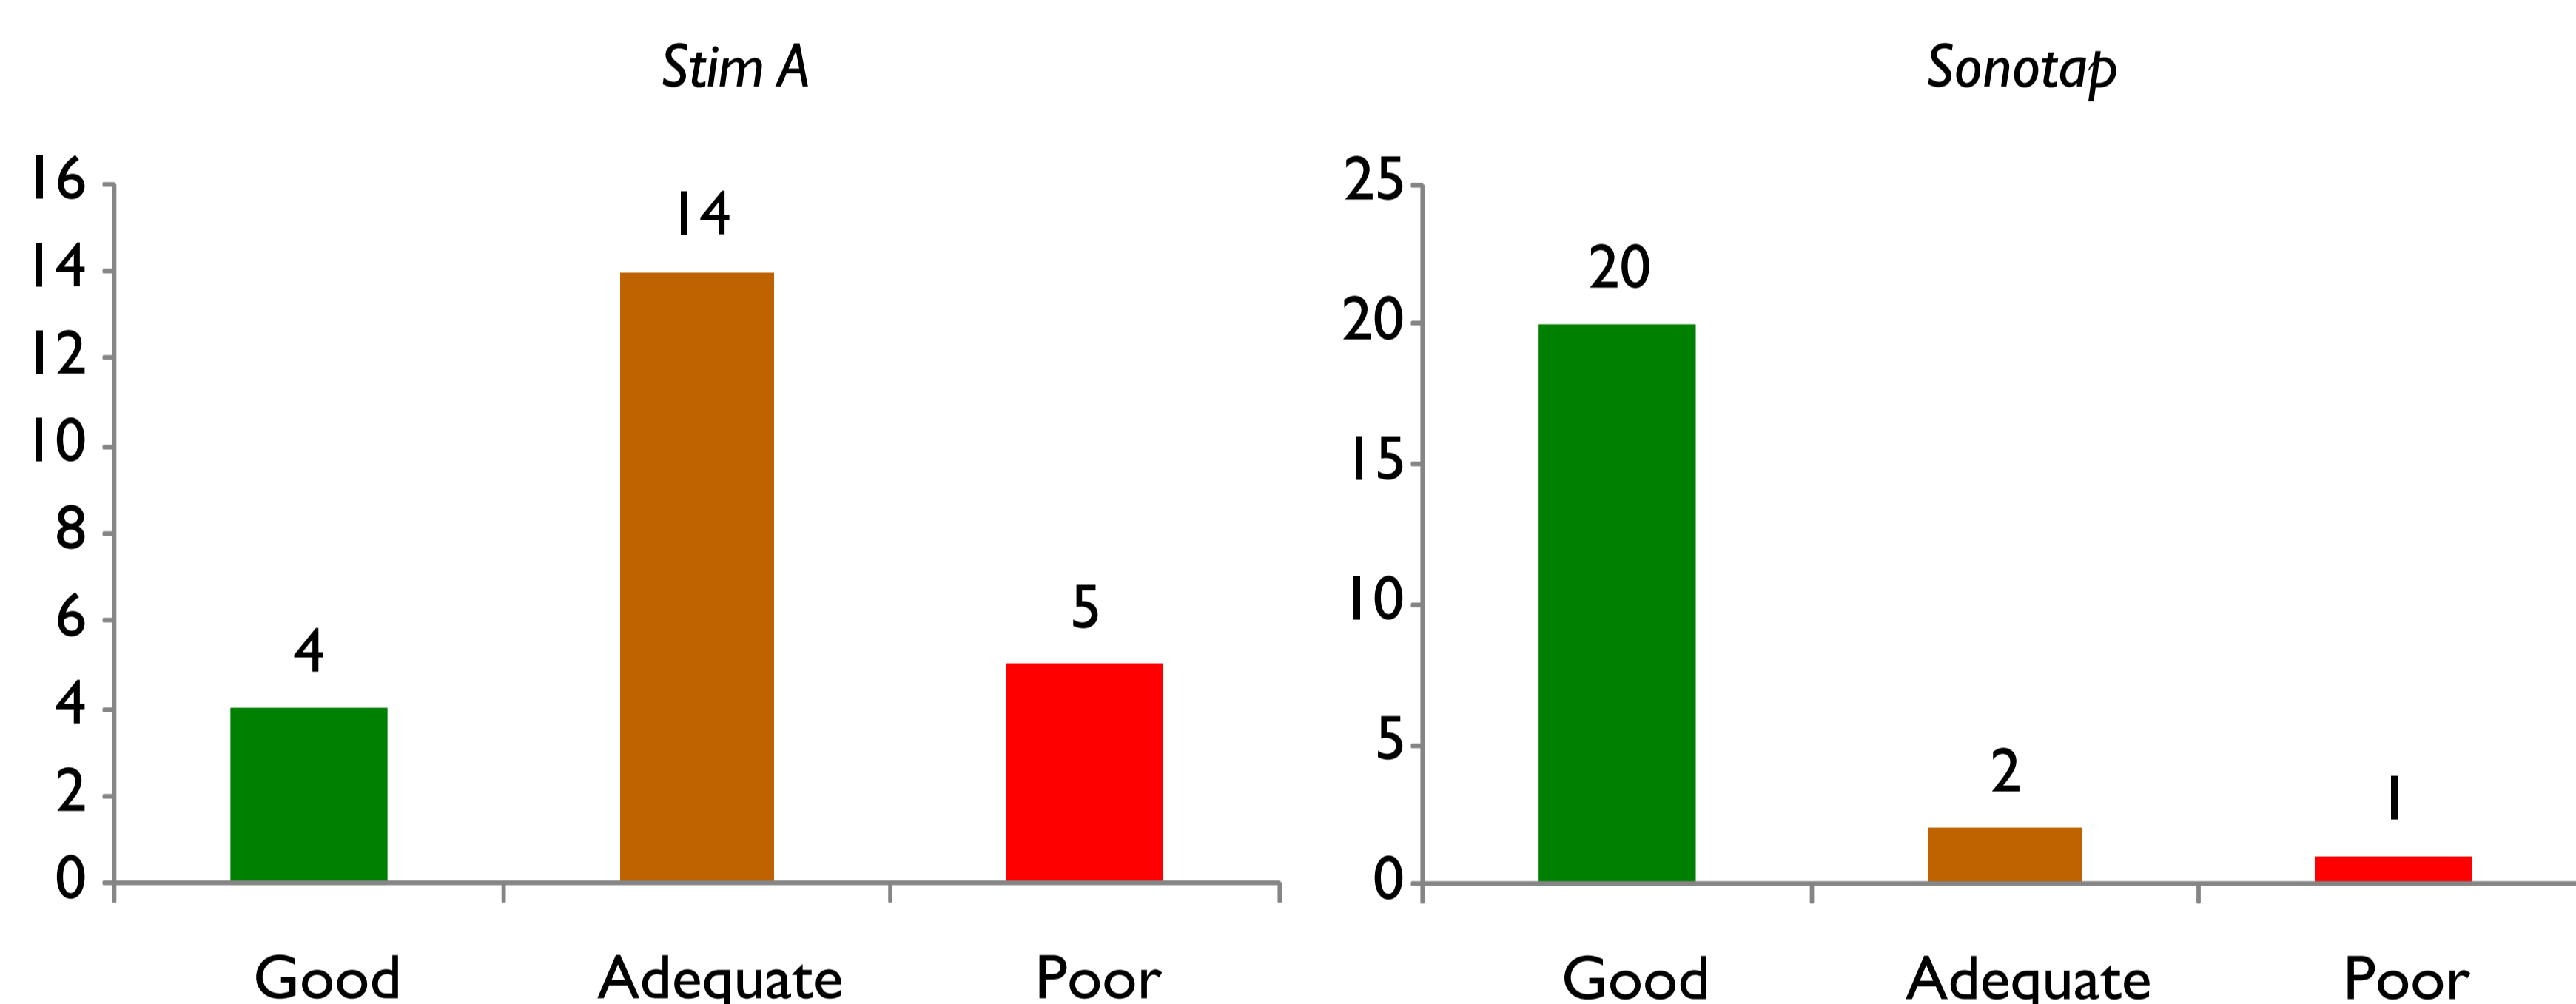

Conclusions

- Our study demonstrated the superiority of the Pajunk Sonotap needle over the other hyperechogenic needle used by the department, the Stimuplex D+.
- Although ranked lower, the MBe mode (present on newer Sonosite machines) enhanced visualisation of the Stimuplex A giving a similar image quality to the Sonotap.
- Therefore we recommend Pajunk hyperechogenic needles or MBe mode with a non-hyperechogenic needle.
- However given the price difference between the needles, the cost savings of using non-hyperechogenic needles should be considered.